

METES 340 REF

High-Precision Meter Test System





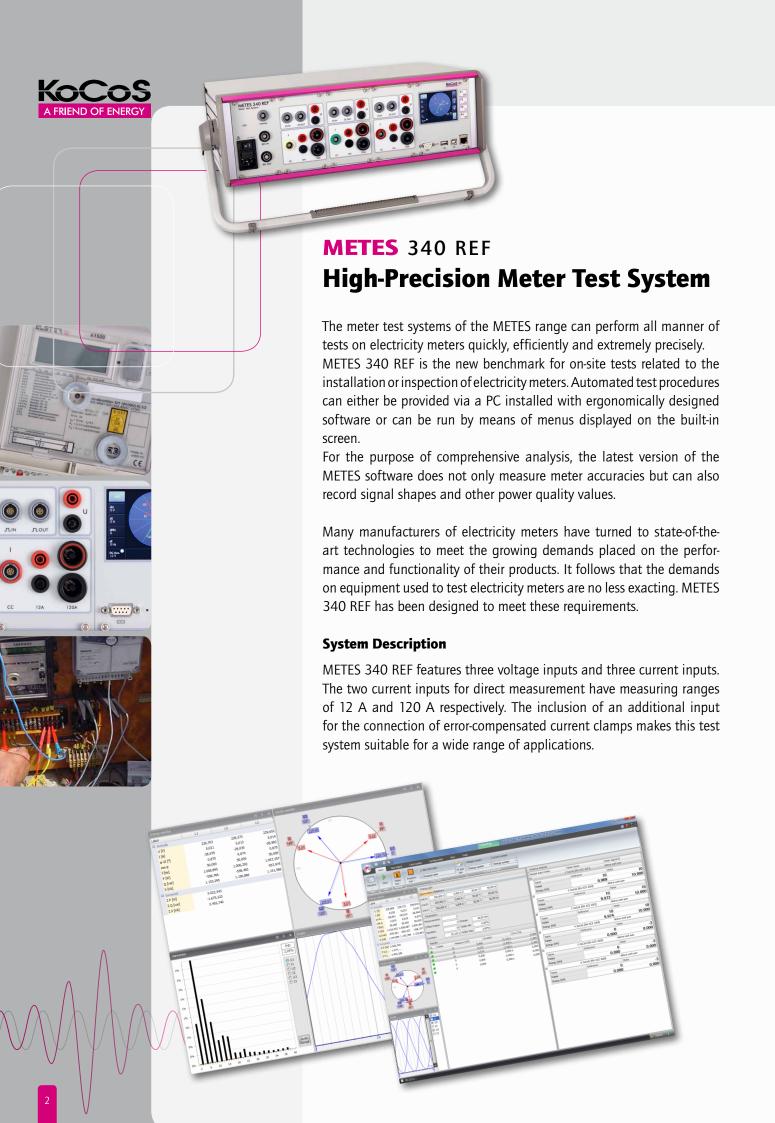

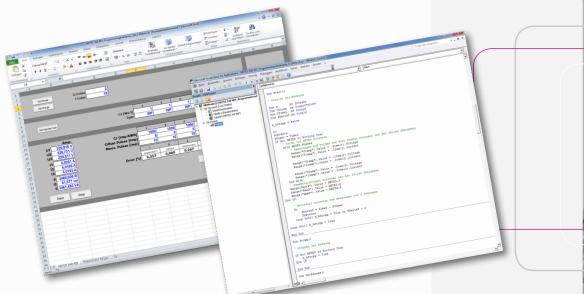

Configurable impulse inputs allow the connection of all commonly used scanning heads. Not only is it possible to select various different input voltages for these inputs, but the meter constant, energy type and impulse length can also be set individually. The same also holds true for the impulse output.

In addition to determining meter accuracy, METES 340 REF can also measure power quality. A multitude of other electrical quantities can be calculated and analysed on the basis of the measured values, including the full complement of power quantities, DC content and harmonics.

Easy to Operate

METES 340 REF can be operated either with a PC and the METES software or alternatively by means of a built-in control panel equipped with a high-resolution, resistive 3½" touch screen and four function keys. The graphical user interface makes for easy, intuitive operation. All the settings required for a test are displayed clearly on the screen.

User-friendly Test Software

A PC or laptop computer can also be connected directly to METES 340 REF. As a result the device can also be operated and controlled via the powerful METES software for manual and automatic tests on electricity meters. Using the software it is easy to create an individual test plan for each test object which can then be run any number of times under identical test conditions.

Test results can either be displayed in the form of fault curves or clearly structured value tables and can also be presented in individually configurable test reports.





F2

F3

F4







In METES 340 REF an active USB interface has been integrated for data transfer via USB storage media, while an Ethernet interface allows direct integration in any network.

Programming Interface

The software also features a simple programming interface with a self-explanatory library for special requirements, e.g. for use with test stands developed by customers for their own use. This programming interface can be used in environments which support COM/ActiveX or in .NET environments.

Analog inputs	Voltage	3 x 0480 VAC
	Direct current	3 x 012 AAC
		3 x 0120 AAC
	Current clamps	3
Accuracy classes	METES 340 REF (0.05)	0.05%
	METES 340 REF (0.02)	0.02%
Impulse inputs	6	Input level up to 24 VDC,
		power supply 12 VDC / 24 VDC
Impulse outputs	6	Proportional to energy
Binary inputs	4	Trigger range 24 to 300 VDC
Binary outputs	3	Potential-free (dry) output relays
Time synchronisation		Internal GPS receiver module
Operation		Touch screen, membrane keypad with 4 function keys, PC
Display		High-resolution, resistive 31/2" touch screen
Communication		RS232, USB-A, USB-B, Ethernet (RJ 45)
Housing (WxHxD) [mm]	470 x 162 x 316	19", 3 HU





KoCoS Messtechnik AG

Suedring 42 D-34497 Korbach, Germany Phone +49 5631 9596-0 Fax +49 5631 9596-17 info@kocos.com www.kocos.com

